



***REFRIGERATION DOES NOT IMPAIR
THE RECOVERY OF NEISSERIA
GONORRHOEAE FROM CHARCOAL
TRANSPORT MEDIUM***

M A Graver & J J Wade

Health Protection Agency London, Department of Medical Microbiology

King's College Hospital, Denmark Hill, London SE5 9RS



King's College Hospital



NHS Trust

REFRIGERATION DOES NOT IMPAIR GONORRHOEAE FROM CHARCOAL

D-1705



M A Graver & J J Wade
Health Protection Agency
London
Department of Medical
Microbiology
King's College Hospital
Denmark Hill
London SE5 9RS

Background

Culture recovery of *Neisseria gonorrhoeae* (NG) remains important for the diagnosis of gonorrhoea, especially in females. 'Bed side' inoculation of media is optimal, but can prove impractical, or impossible, in some healthcare settings¹. Despite emergent molecular diagnostics, the need to recover NG for susceptibility testing and epidemiological typing ensures that transport media remain indispensable in the management of gonorrhoea. This is underscored by the development of an NCCLS quality control standard for microbiological transport systems (M-40).

Although many evaluations of media and 'transport systems' have been made, it remains unclear whether refrigeration of transport swabs improves, or is detrimental to, the recovery of NG. To address this we measured the survival of 30 distinguishable strains of NG at room temperature (RT) and at 4°C. We also evaluated the effects of two suspending media for the preparation of the inocula in these experiments.

Methods

Thirty clinical isolates of NG, distinguishable by auxotyping, epidemiologically, or both were studied. For each strain two inocula were prepared. Initially a 2 mL suspension in phosphate-buffered saline (PBS, Sigma-Aldrich, Poole, UK) was prepared to a McFarland No. 1 standard; 0.5 mL of this was added to 0.5 mL of PBS (PBS inoculum), and 0.5 mL to 0.5 mL of nutrient broth (Oxoid, Basingstoke, UK; PBS:broth inoculum). Swabs were inoculated with 100µL of suspensions.

'Transwab®' rayon-tipped swabs with plastic shafts and charcoal-containing Amies medium (Medical Wire & Equipment Co, Corsham, UK) were used throughout. For each strain, eight swabs were inoculated, to allow

comparison of all combinations of: the PBS or PBS:broth inocula; storage at RT or 4°C; for 24 or 48h.

At times 24h and 48h, NG were recovered from swabs by vortexing the tips in 1mL PBS for 30s. Triplicate counts were performed on the time 0h inocula and washings, using a spiral plater (Don Whitley, Shipley, UK), on chocolate agar (Oxoid, Basingstoke, UK). For each of the 30 strains, the median of the three counts was taken for each of the eight possible inoculum / medium / time interval combinations.

Results

Figures 1 & 2. The median log counts at time 0h for the PBS and PBS:broth inocula were 6.68 and 6.48, respectively (P=NS). At 48h the recovery from swabs held at 4°C was significantly better than for those held at RT, but only for the inoculum prepared in PBS rather than PBS:broth.

Discussion

Cooling specimens – including the use of dry ice² - to preserve gonococci during transport has been considered for many years. Although Stuart *et al* recommended refrigerating Stuart's transport medium in 1954³, they provided no evidence to support this, and Stuart did not suggest refrigeration in his original paper⁴. Amies gave no recommendation about holding temperatures for his modification of Stuart's medium⁵. Stuart's and Amies' media may even differ in this respect: in a study of urethral pus from 58 men inoculated on to (rather than in to) three semi-solid transport media, Taylor & Phillips found that storage at 4°C improved recovery of gonococci from Stuart's, but not Amies', medium⁶.

Our study includes more strains of GC than other *in vitro* evaluations to date. Sng *et al*, in a semiquantitative study, looked at the survival of 5 strains of NG in Amies at four temperatures (4, 18, 26 & 32°C) and found better survival at lower temperatures up to 48h⁷. Arbique *et al*, studying six isolates found that recovery was improved by refrigeration, though optimum temperature varied with transport system⁸. Perry *et al*⁹, using three isolates, considered that 4°C prolonged survival. In

THE RECOVERY OF NEISSERIA GONORRHOEA IN COAL TRANSPORT MEDIUM

other studies of NG ATCC 43069, in various transport systems, recovery has usually been improved by storage at 4°C¹⁰⁻¹², though not always¹³.

Figure 1. Phosphate-buffered saline Inoculum


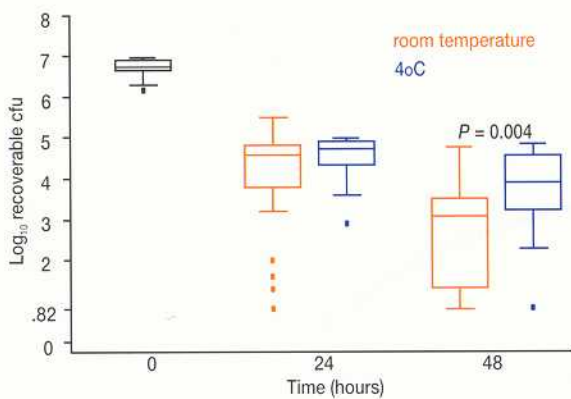


Figure 2. 50:50 phosphate-buffered saline : broth mix inoculum

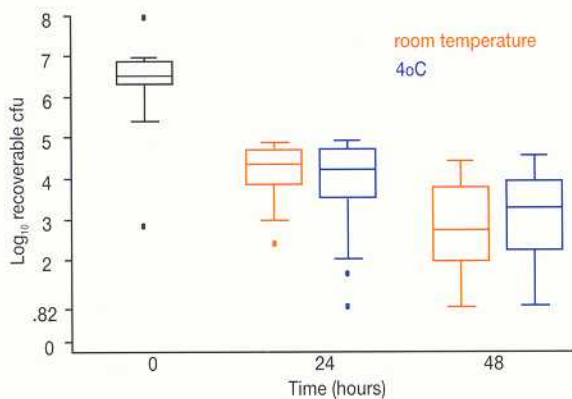

Conclusions

Our results add to a growing body of evidence that refrigeration does not reduce the yield of NG and may be beneficial. This is in keeping with observations that NG autolysis is minimal at lower temperatures¹⁴⁻¹⁶. Further studies – using fresh clinical isolates – are needed to determine the degree to which survival of NG in different commercially available systems is affected by temperature. We found that the type of inoculum used - PBS or PBS:broth - affected our results: standardising the menstruum used for the inocula in quality control testing (as proposed by the approved NCCLS M-40) is essential.

Acknowledgements

Medical Wire & Equipment Co Ltd (MG)

AstraZeneca UK (MG, JW)

The Special Trustees, King's College Hospital (MG:
King's Development Award)

M A Graver & J J Wade

Health Protection Agency London, Medical Microbiology

King's College Hospital, Denmark Hill, London SE5 9RS


Tel: +44 2073463033 Fax: +44 2073463404

Michelle.graver@kingsch.nhs.uk

jimwade@btinternet.com

References

1. Olsen, C.C., Schwebke, J.R., Benjamin, W.H., Beverly, A., and K. B. Waites. Comparison of direct inoculation and Copan transport systems for isolation of *Neisseria gonorrhoeae* from endocervical specimens. *J. Clin. Microbiol* 1999;**37**:3583-3585.
2. Sanderson ES, Allison GG. The use of dry ice in the shipment of material for gonococcal cultivation. *Amer J Syph* 1942;**26**:196-200.
3. Stuart RD, Toshach SR, Patsula TM. The problem of transport of specimens for culture of gonococci. *Can J Pub Hlth* 1954;**45**:73-83.
4. Stuart RD. The diagnosis and control of gonorrhoea by bacteriological cultures. *Glas Med J* 1946;**27**:131-142.
5. Amies C, R. 1967. A modified formula for the preparation of Stuart's transport medium. *Can. J. Public Health* 1967;**58**:296-300.
6. Taylor E, Phillips I. Assessment of transport and isolation methods for gonococci. *Br J Ven Dis* 1980;**56**:390-393.
7. Sng E, Rajan VS, Yeo K, Goh A. The recovery of *Neisseria gonorrhoeae* from clinical specimens: effects of different temperatures, transport times, and media. *Sex Transm Dis* 1982; **9**:74-78.
8. Arbique JC, Forward KR, LeBlanc J. Evaluation of four commercial transport media for the survival of *Neisseria gonorrhoeae*. *Diagn Microbiol Infect Dis* 2000;**36**:163-168.
9. Perry JL. Effects of temperature on fastidious organism viability during swab transport. 101st ASM General Meeting, Orlando, 2001.
10. Robinson A, Gruver ML. Comparison of bacterial survival in two transport systems stored at room and refrigerator temperatures. ASM 102nd General Meeting, Salt Lake City, 2002.
11. Sarina M, Knoll B. Comparative study of two transport systems (Copan Easy-Flow and Starplex STARSWAB II) using the roll-plate and vortex methods, following incubation at room temperature and 4°C. ASM 102nd General Meeting, Salt Lake City, 2002.
12. Mitchell E, Berman M, Ginocchio CC. Evaluation of two new liquid Stuart swab transport systems: platinum Starswab II (Starplex scientific) and BBL Cultureswab (Becton Dickinson). ASM 102nd General Meeting, Salt Lake City, 2002.
13. Rousee JM, Hernandez C, DeMartino S, Zachary P, Monteil H, Piedmont Y. Comparison of four swab transport systems stored at room temperature and +4°C for recovery of previously inoculated fastidious aerobic and anaerobic bacteria. 101st ASM General Meeting, Orlando, 2001.
14. Hebel BH, Young FE. Autolysis of *Neisseria gonorrhoeae*. *J Bacteriology* 1975;**122**:385-392.
15. Elmros T, Burman LG, Bloom GD. Autolysis of *Neisseria gonorrhoeae*. *J Bacteriology* 1976;**126**:969-976.
16. Elmros T, Sandstrom G, Burman L. Autolysis of *Neisseria gonorrhoeae*. Relation between mechanical stability and viability. *Brit J Vener Dis* 1976;**52**:246-249.

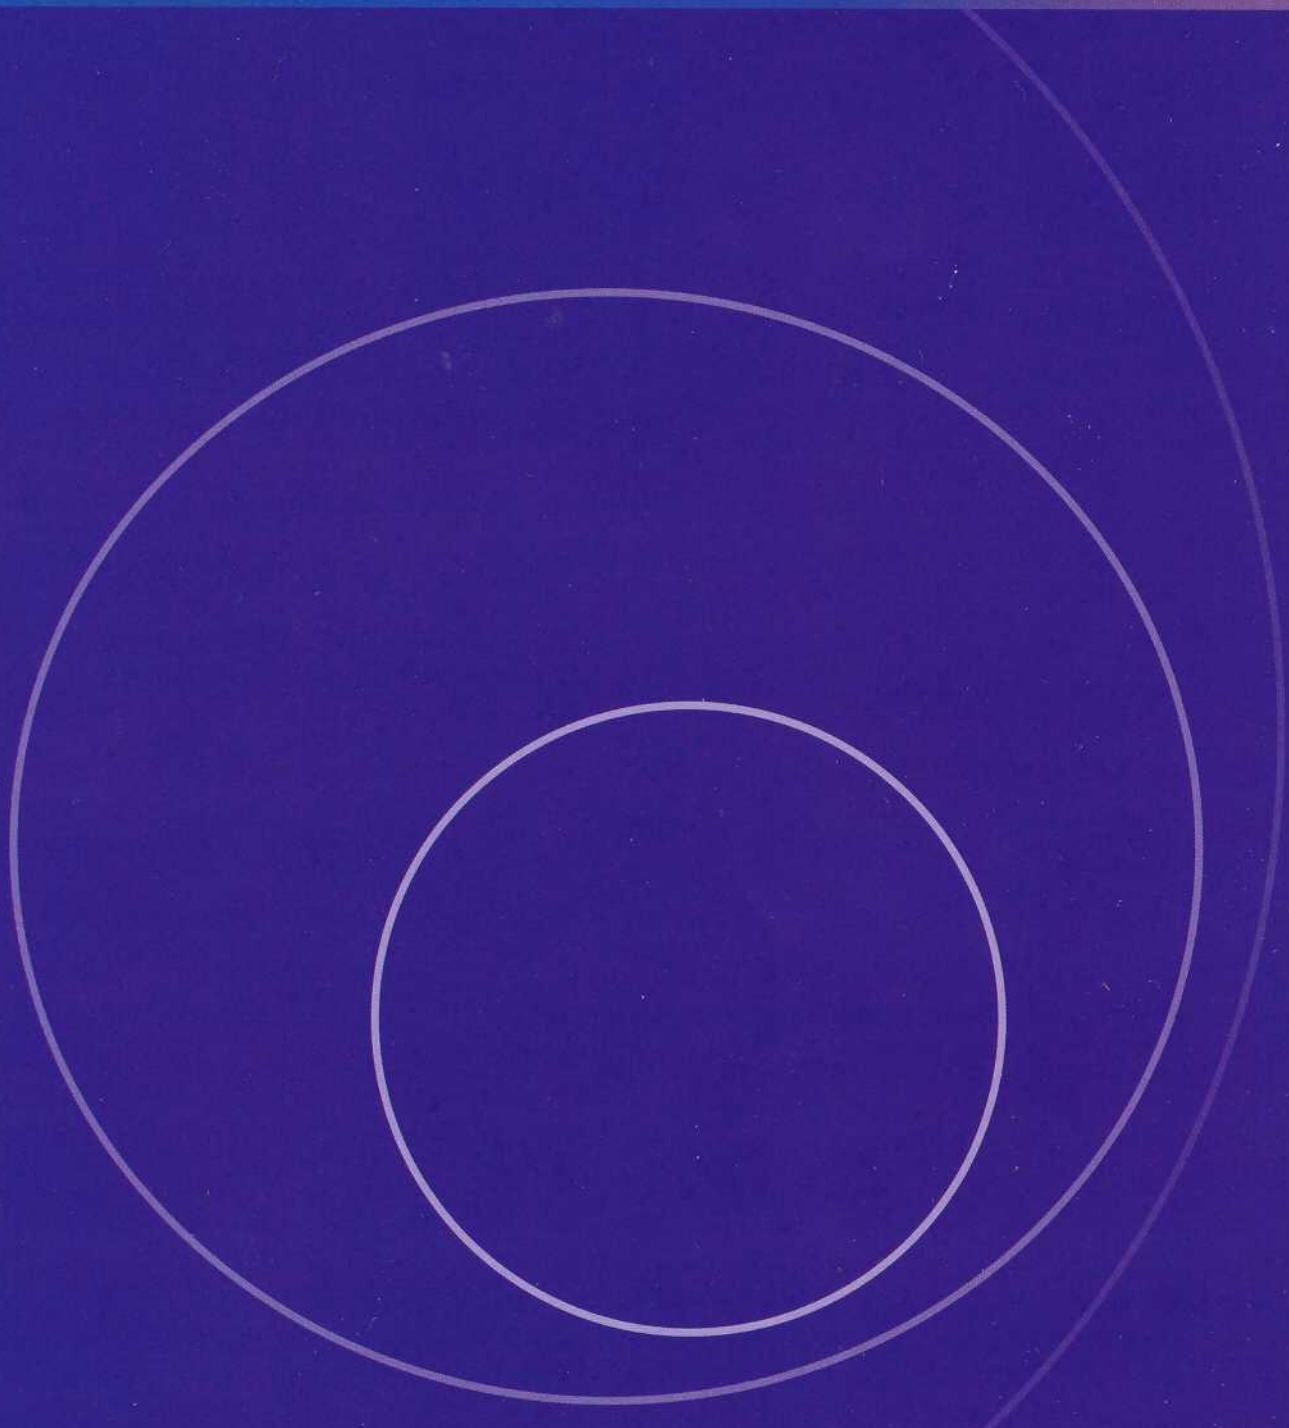

Medical Wire & Equipment

Corsham, Wiltshire, England SN13 9RT

Telephone: +44(0)1225 810361 Fax: +44(0)1225 810153

E-mail: info@mwe.co.uk Website: www.mwe.co.uk